


Dressler FD-557
188 g/mol, 12mg


7.14 7.13 7.12 7.10 7.10 7.10 7.08 7.08 7.07 7.07 7.06 7.05 6.98 6.99 6.99 6.99 6.97 6.97 6.97 6.97 6.97 5.24 5.23 5.23 2.94 2.93 2.93 2.25 2.21 2.21 2.20 2.19 2.17 2.16 2.15 2.14 1.99 1.99 1.97 1.95 1.90 1.90 1.89 1.89 1.88 1.88 1.87 1.86 1.86 1.47 1.46 1.46 1.45 1.44 1.43 1.43 1.41 1.40 1.39 1.37 1.25 1.23 1.23

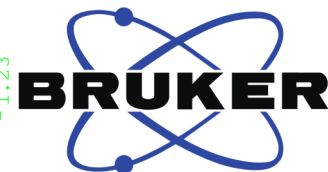

Current Data Parameters
NAME FDSep06-2023HD
EXPNO 40
PROCNO 1

F2 - Acquisition Parameters
Date_ 20230906
Time 8.40 h
INSTRUM spect
PROBHD Z125339_0010 (
PULPROG zg30
TD 65536
SOLVENT CD2Cl2
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.122266 Hz
AQ 4.0894465 sec
RG 200.5
DW 62.400 usec
DE 6.50 usec
TE 298.1 K
D1 1.00000000 sec
TD0 1
SFO1 400.2524715 MHz
NUC1 1H
P1 15.00 usec
PLW1 25.02099991 W

F2 - Processing parameters
SI 65536
SF 400.2500505 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

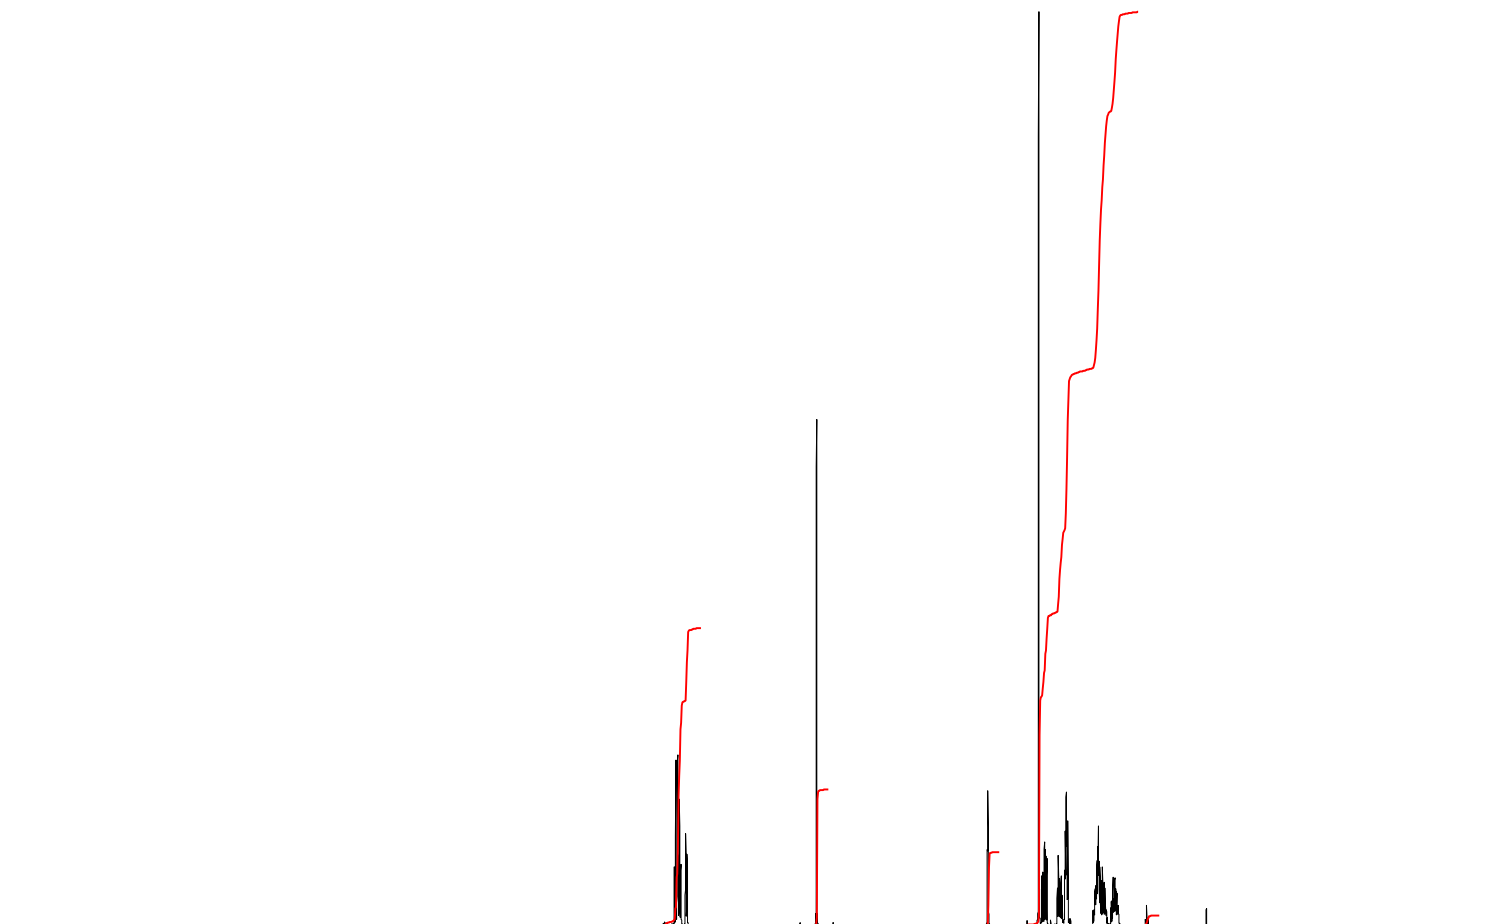

15 14 13 12 11 10 9 8 7 6 5 4 3 2 1 0 -1 -2 ppm

20.79 9.51 5.15 63.82 0.73