


Dressler FD-549


242 g/mol / 18 mg

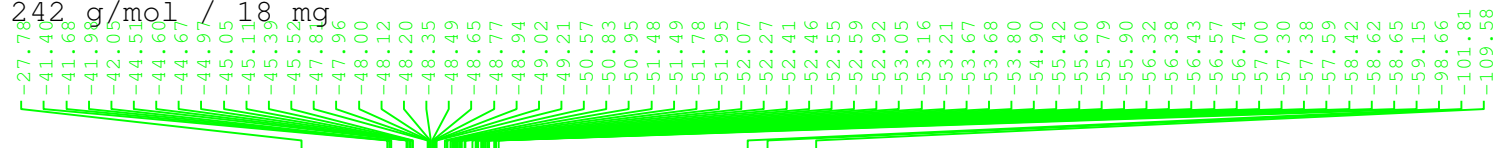

Current Data Parameters
NAME FDSep04-2023HD
EXPNO 271
PROCNO 1

F2 - Acquisition Parameters
Date_ 20230904
Time 9.53 h
INSTRUM spect
PROBHD Z125339_0010 (
PULPROG zgfhigqn.2
TD 131072
SOLVENT CD2Cl2
NS 256
DS 4
SWH 89285.711 Hz
FIDRES 0.681196 Hz
AQ 0.7340032 sec
RG 200.5
DW 5.600 usec
DE 6.50 usec
TE 298.6 K
D1 1.00000000 sec
D11 0.03000000 sec
D12 0.00002000 sec
TD0 1
SFO1 376.5736179 MHz
NUC1 19F
P1 22.00 usec
PLW1 26.57399940 W
SFO2 400.2516010 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 25.02099991 W
PLW12 0.70070952 W

F2 - Processing parameters
SI 65536
SF 376.6112790 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

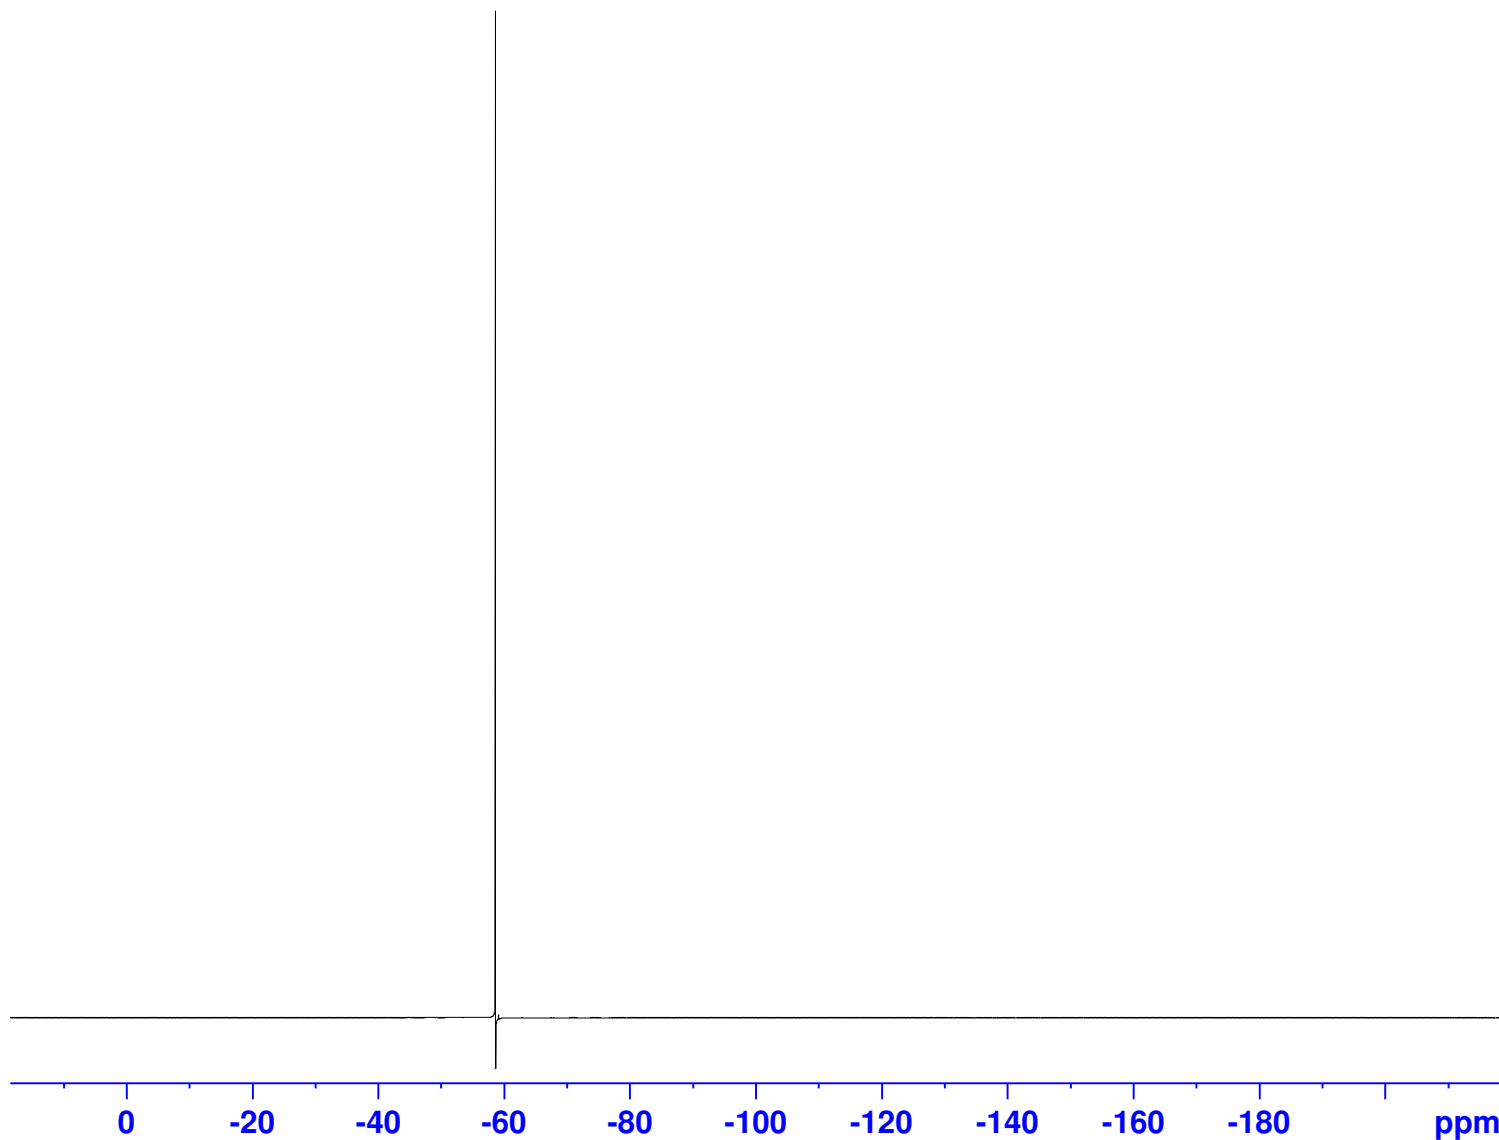

7.50
2.50