

Dressler FD-550
242 g/mol / 20 mg


7.55
7.51
7.49
7.46
7.43
7.40
7.38
7.37
5.23
5.23
5.23
2.95
2.95
2.94
2.25
2.23
2.23
2.21
2.20
2.19
2.17
2.03
2.02
2.01
2.00
1.99
1.98
1.92
1.92
1.91
1.90
1.89
1.89
1.88
1.52
1.51
1.50
1.50
1.49
1.49
1.48
1.48
1.47
1.46
1.46
1.44
1.44
1.44
1.43
1.43
1.41
1.41
1.41
1.40
1.39
1.28
1.27
1.26
1.25
1.24
1.23
1.22
-0.00



Current Data Parameters
NAME FDSep04-2023HD
EXPNO 280
PROCNO 1

F2 - Acquisition Parameters
Date_ 20230904
Time 16.22 h
INSTRUM spect
PROBHD Z125339_0010 (
PULPROG zg30
TD 65536
SOLVENT CD2Cl2
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.122266 Hz
AQ 4.0894465 sec
RG 200.5
DW 62.400 usec
DE 6.50 usec
TE 298.0 K
D1 1.00000000 sec
TD0 1
SFO1 400.2524715 MHz
NUC1 1H
P1 15.00 usec
PLW1 25.02099991 W

F2 - Processing parameters
SI 65536
SF 400.2500506 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

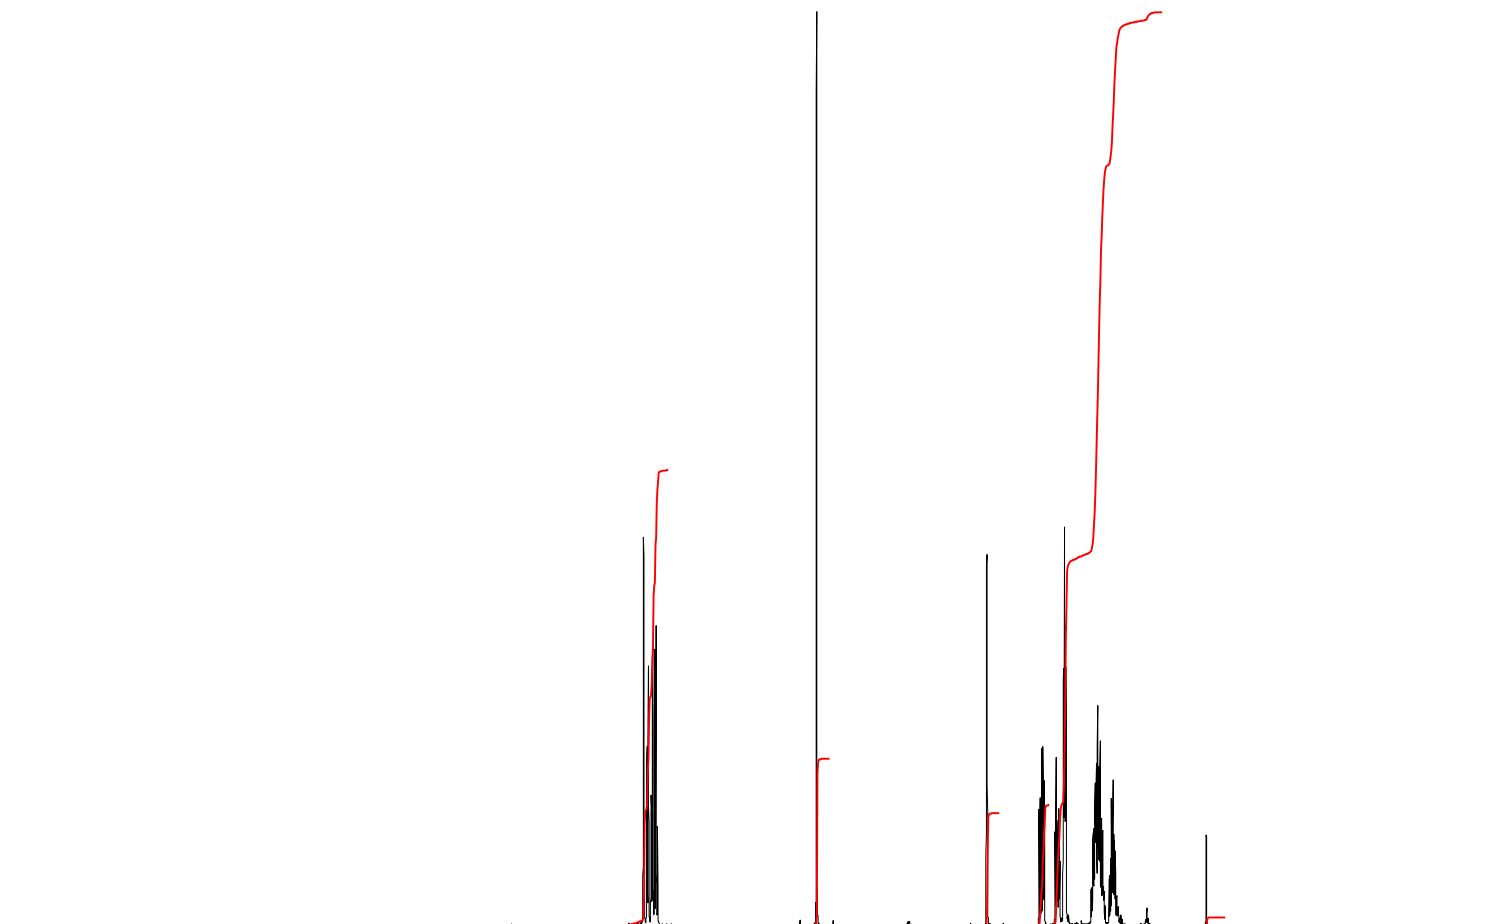

15 14 13 12 11 10 9 8 7 6 5 4 3 2 1 0 -1 -2 ppm

25.63
9.40
6.34
6.79
51.36
0.48