



Dressler FD-512  
477 g/mol / 30 mg

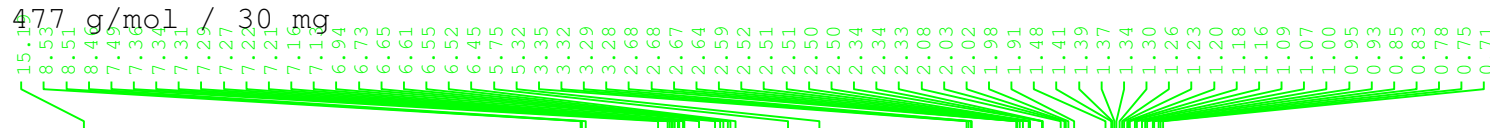

Current Data Parameters  
NAME FDAug22-2023HD  
EXPNO 40  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20230822  
Time 16.19 h  
INSTRUM spect  
PROBHD Z125339\_0010 (  
PULPROG zg30  
TD 65536  
SOLVENT DMSO  
NS 16  
DS 2  
SWH 8012.820 Hz  
FIDRES 0.122266 Hz  
AQ 4.0894465 sec  
RG 200.5  
DW 62.400 usec  
DE 6.50 usec  
TE 299.0 K  
D1 1.00000000 sec  
TD0 1  
SFO1 400.2524715 MHz  
NUC1 1H  
P1 15.00 usec  
PLW1 25.02099991 W

F2 - Processing parameters  
SI 65536  
SF 400.2500000 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00

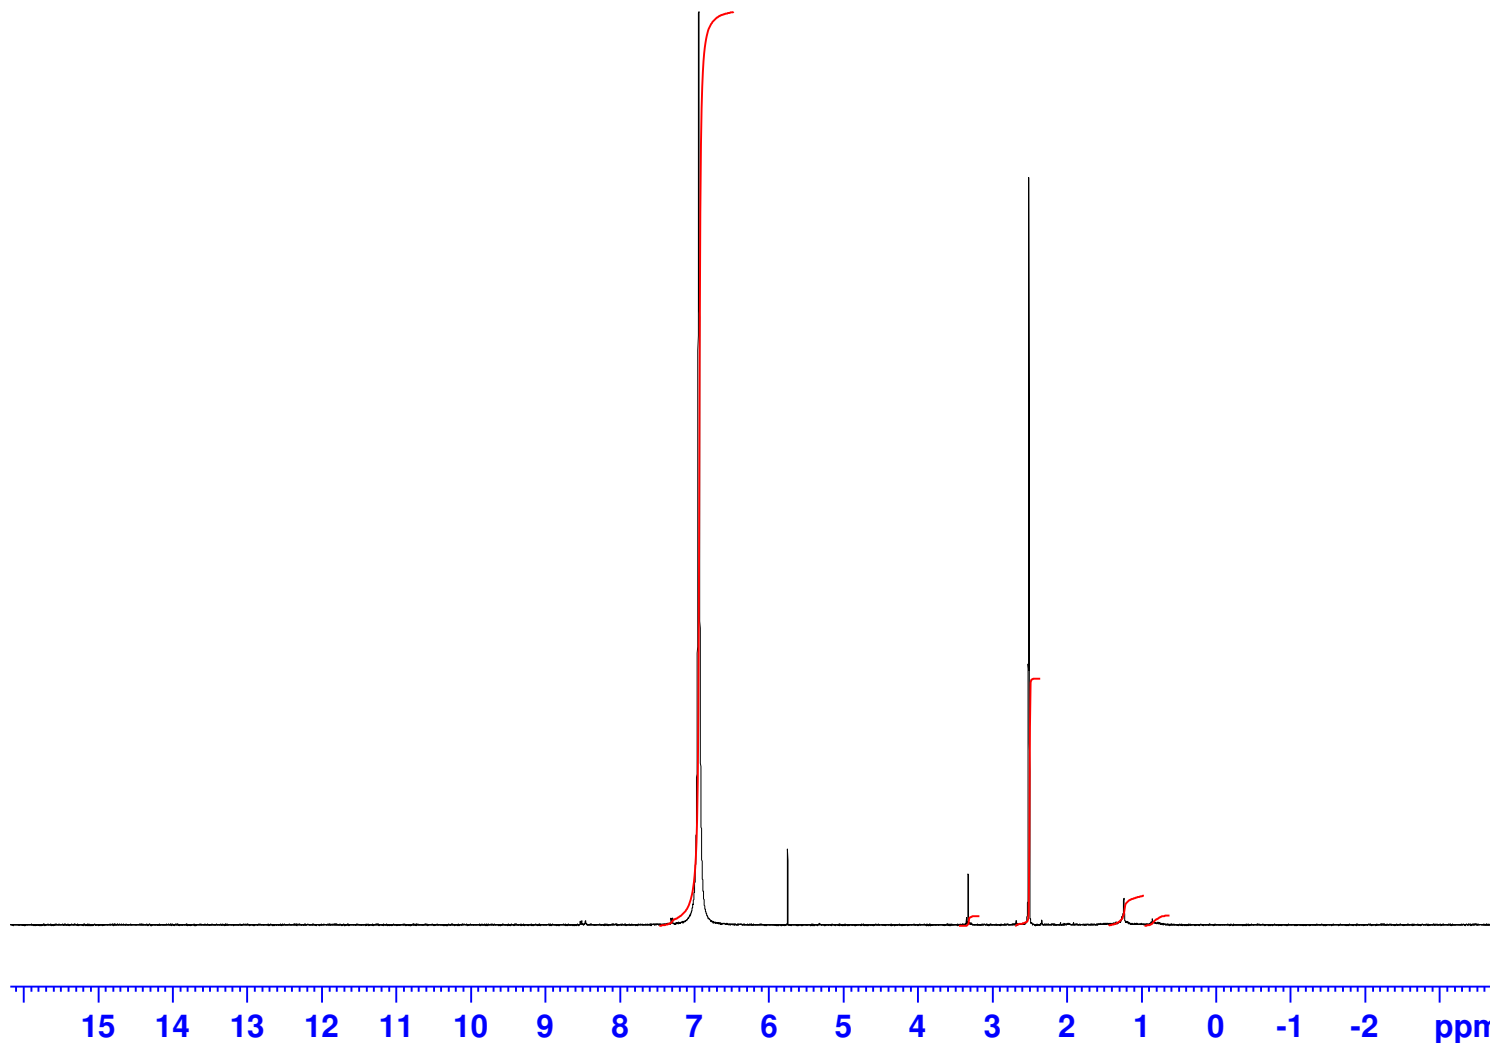

75.49  
0.77  
20.38  
2.49  
0.86