


Mardyukov AMN-S-101.2


7.45
7.20
6.93
6.19
6.18
6.17
6.01
5.99
5.98
5.97
5.97
5.77
5.76
5.75
5.45
5.23
4.06
4.04
3.65
2.81
2.64
2.64
2.63
2.63
2.57
2.52
2.52
2.51
2.45
2.20
2.18
2.11
1.98
1.84
1.81
1.75
1.67
1.61
1.58
1.58
1.57
1.57
1.56
1.56
1.55
1.55
1.54
1.40
1.36
1.26
1.24
1.24
1.21
1.19
1.17
1.15
0.81
0.10
0.02
0.02
0.01
-0.00
-0.01

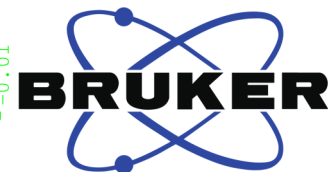

Current Data Parameters
NAME AMJun30-2020HD
EXPNO 120
PROCNO 1

F2 - Acquisition Parameters
Date_ 20200630
Time 21.50 h
INSTRUM spect
PROBHD Z125339_0010 (
PULPROG zg30
TD 65536
SOLVENT CDC13
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.122266 Hz
AQ 4.0894465 sec
RG 200.5
DW 62.400 usec
DE 6.50 usec
TE 298.6 K
D1 1.00000000 sec
TD0 1
SFO1 400.2524715 MHz
NUC1 1H
P1 15.00 usec
PLW1 25.02099991 W

F2 - Processing parameters
SI 65536
SF 400.2500353 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

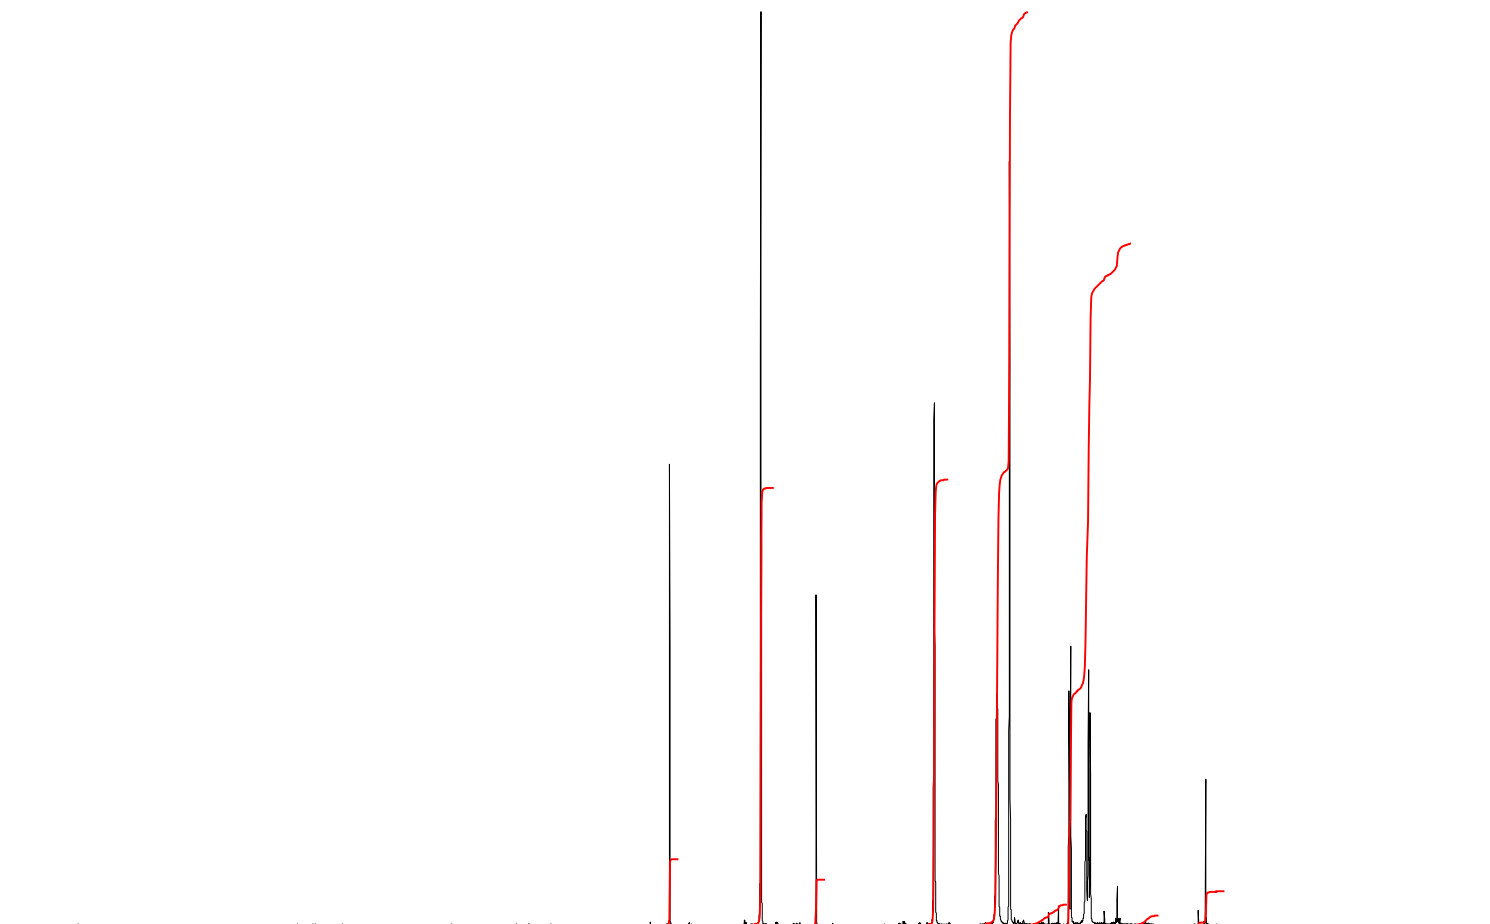

15 14 13 12 11 10 9 8 7 6 5 4 3 2 1 0 -1 -2 ppm

2.49
16.47
1.72
16.81
34.38
0.79
25.68
0.38
1.29